


- **Sonden-Paradibtineter-Kombination**
- **Combination explorer-probes**
- **Sondes-explorateurs**
- **Sondas-exploradores**
- **Combinazioni sonde - Sonde millimetriche paradontali**

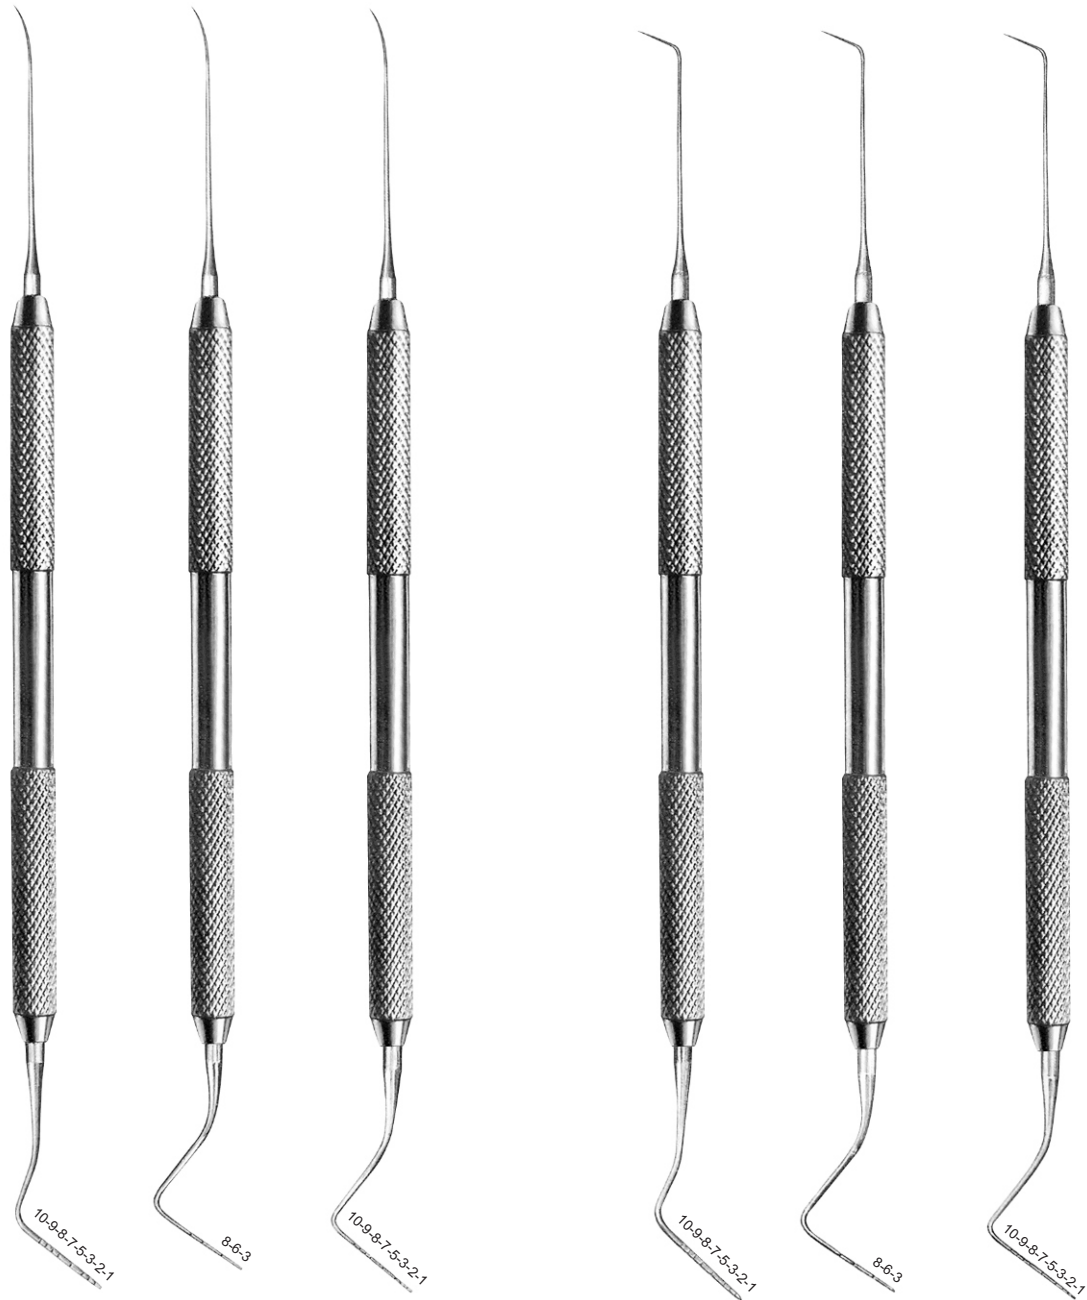

PI-895-015
Fig. 3
Goldman-Fox

PI-895-016
Fig. 3
University of Michigan

PI-895-017
Fig. 3
Williams

PI-895-018
Fig. 16
Goldman-Fox

PI-895-019
Fig. 16
University of Michigan

PI-895-020
Fig. 16
Williams

- **Sonden-Paradibtneter-Kombination**
- **Combination explorer-probes**
- **Sondes-explorateurs**
- **Sondas-exploradores**
- **Combinazioni sonde - Sonde millimetriche parodontali**

